

Fig. 1a

FIG. 1 is a perspective view of a medical device 102. The device includes a handle 110, a shaft 130, and a distal tip 150. A bracket 140 is positioned around the shaft. A label 135 points to a feature on the shaft. A label 102 is at the bottom right.

**Fig.1b**

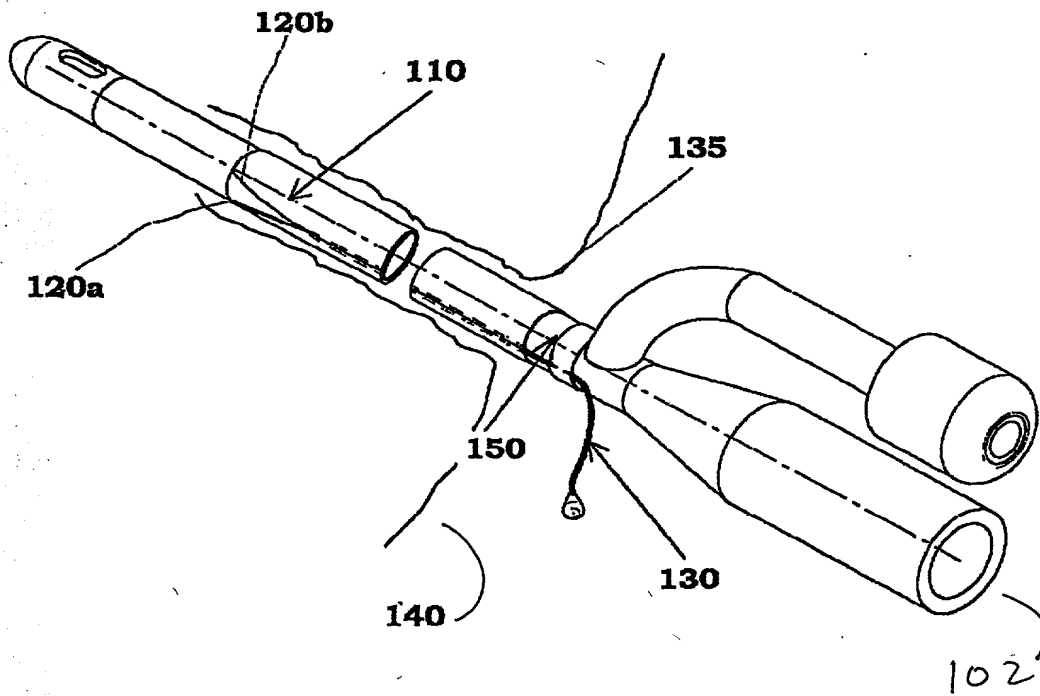


Fig. 1c




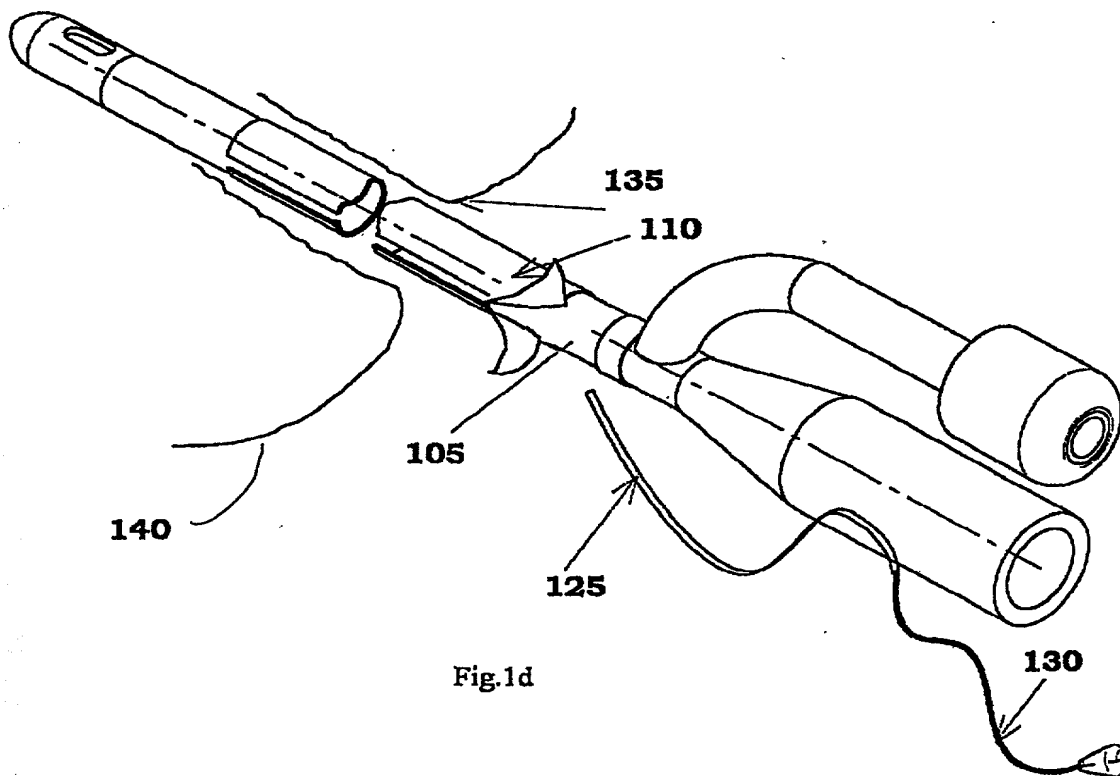


Fig. 1d

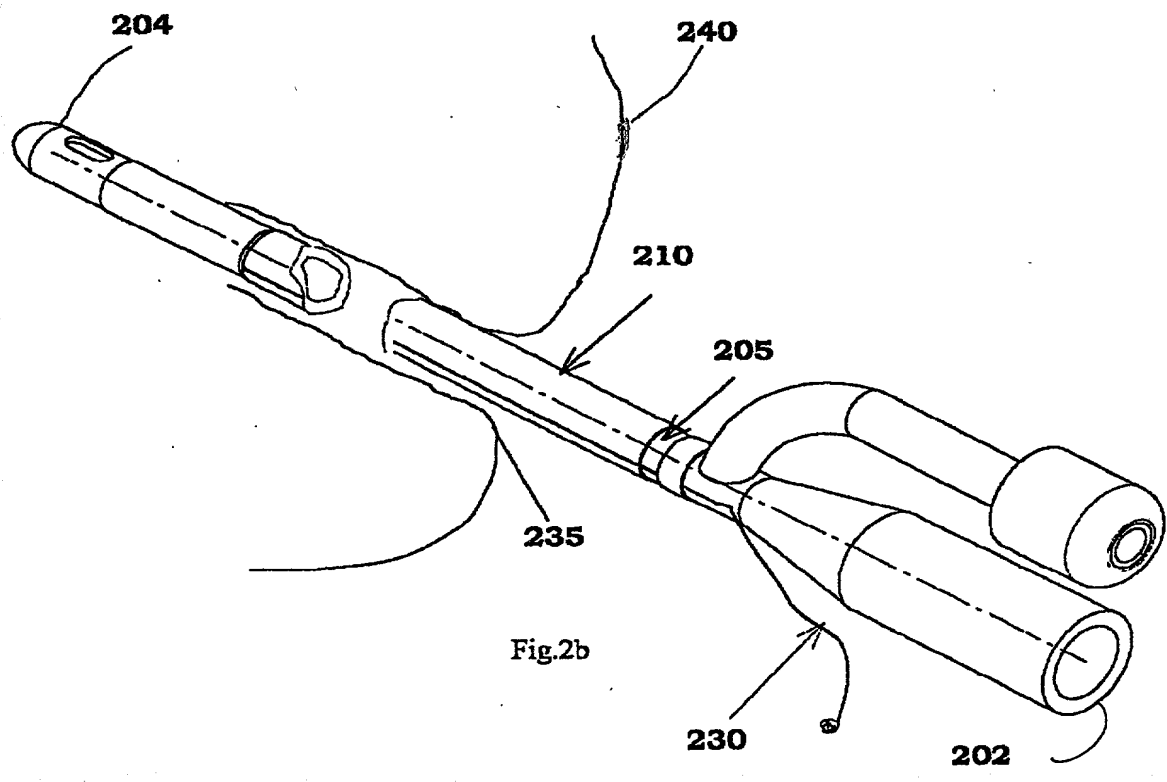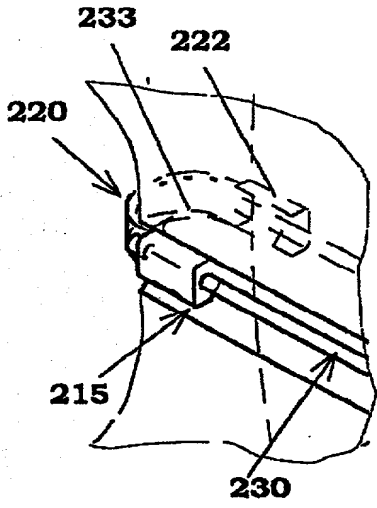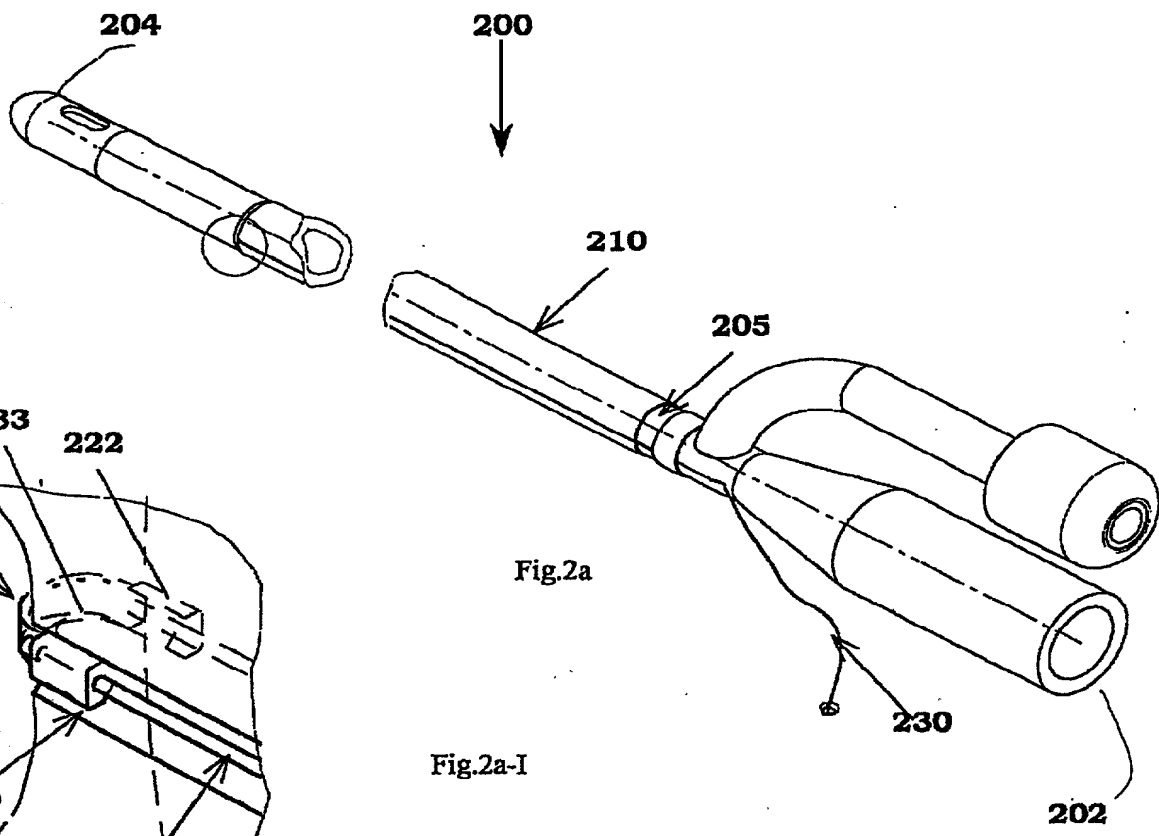

20040704001

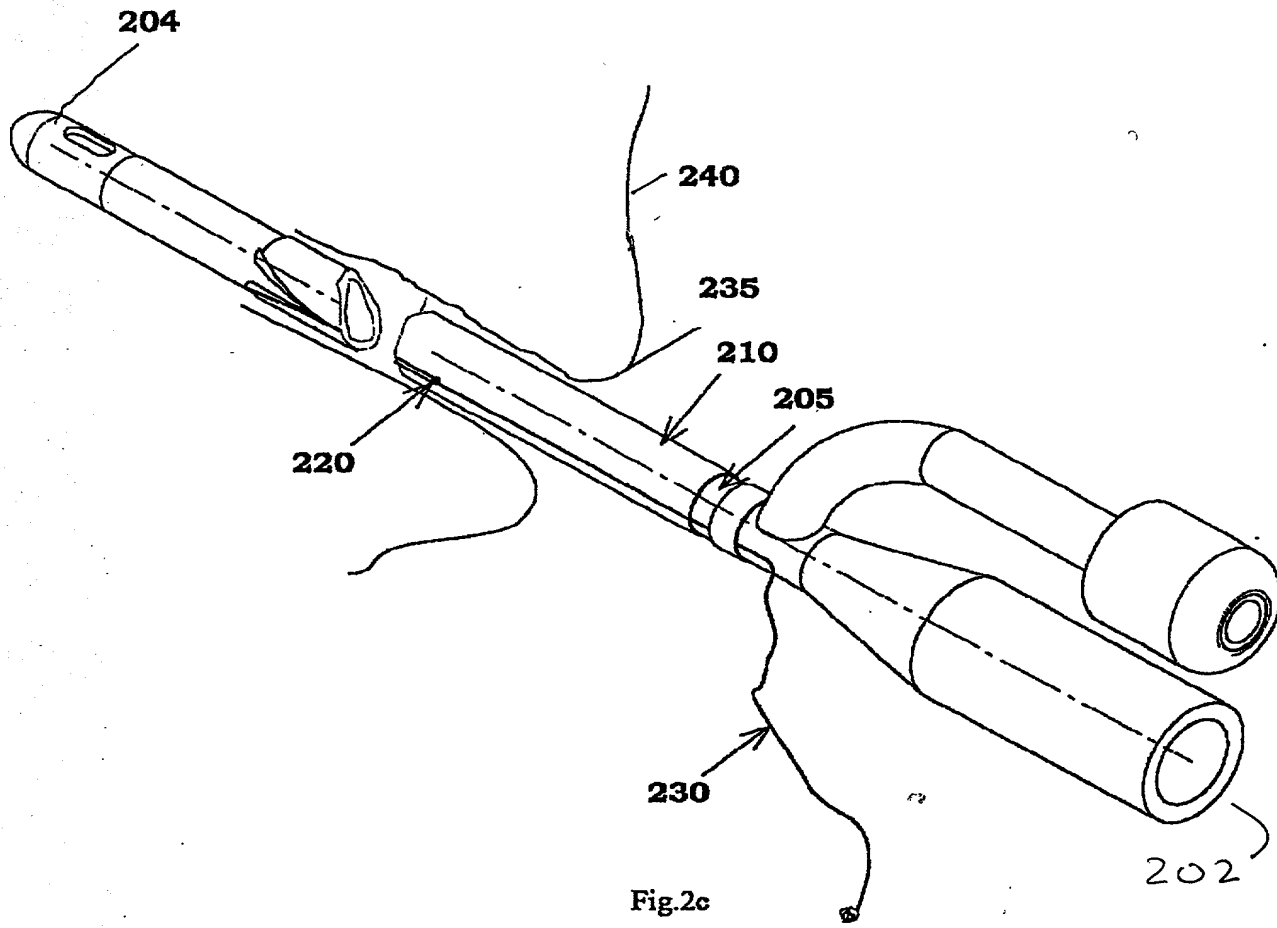


Fig. 2c

4347-001-0000

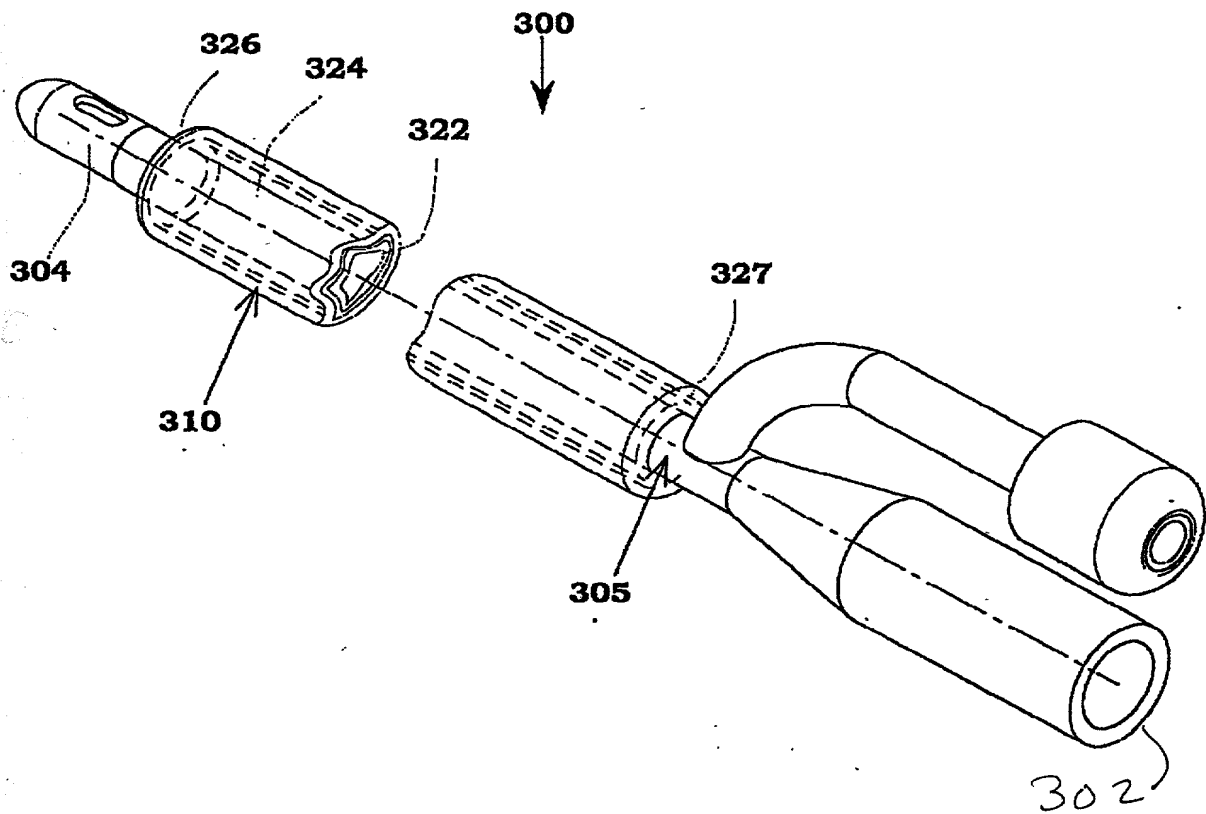


Fig.3a

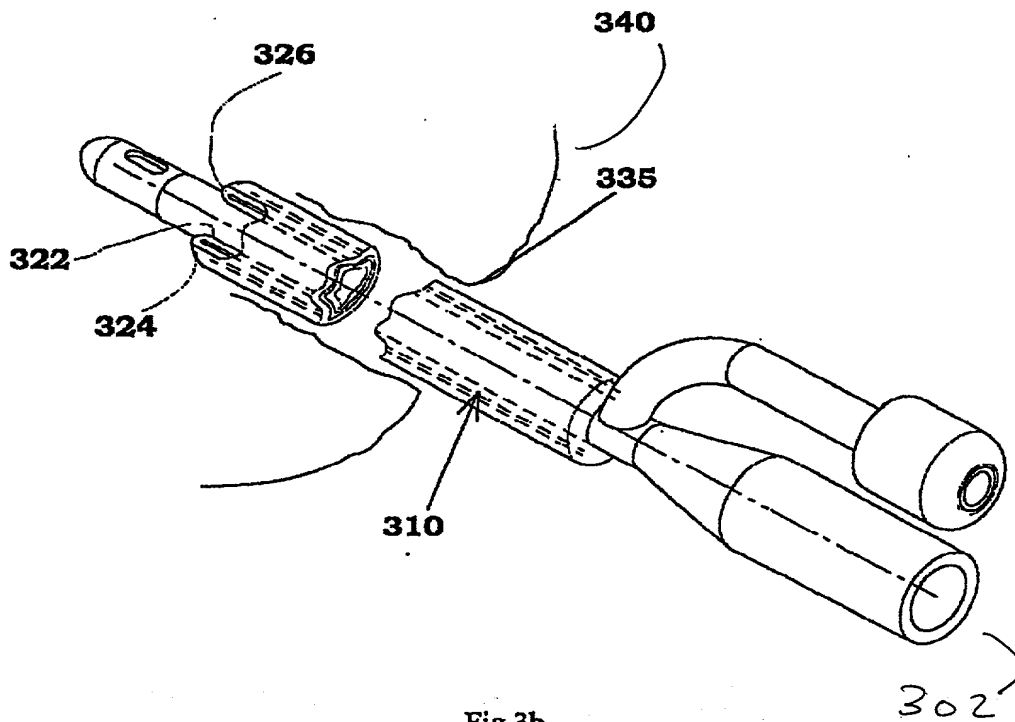


Fig.3b

2007-03-20 14:00:00

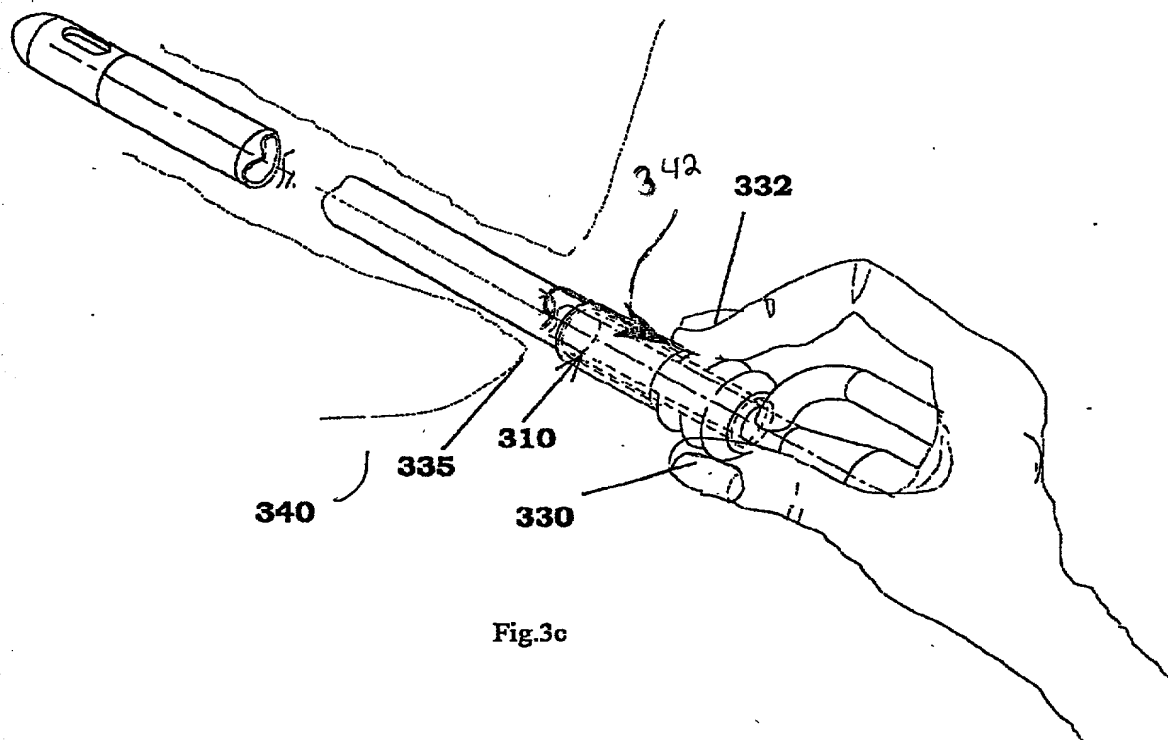


Fig.3c

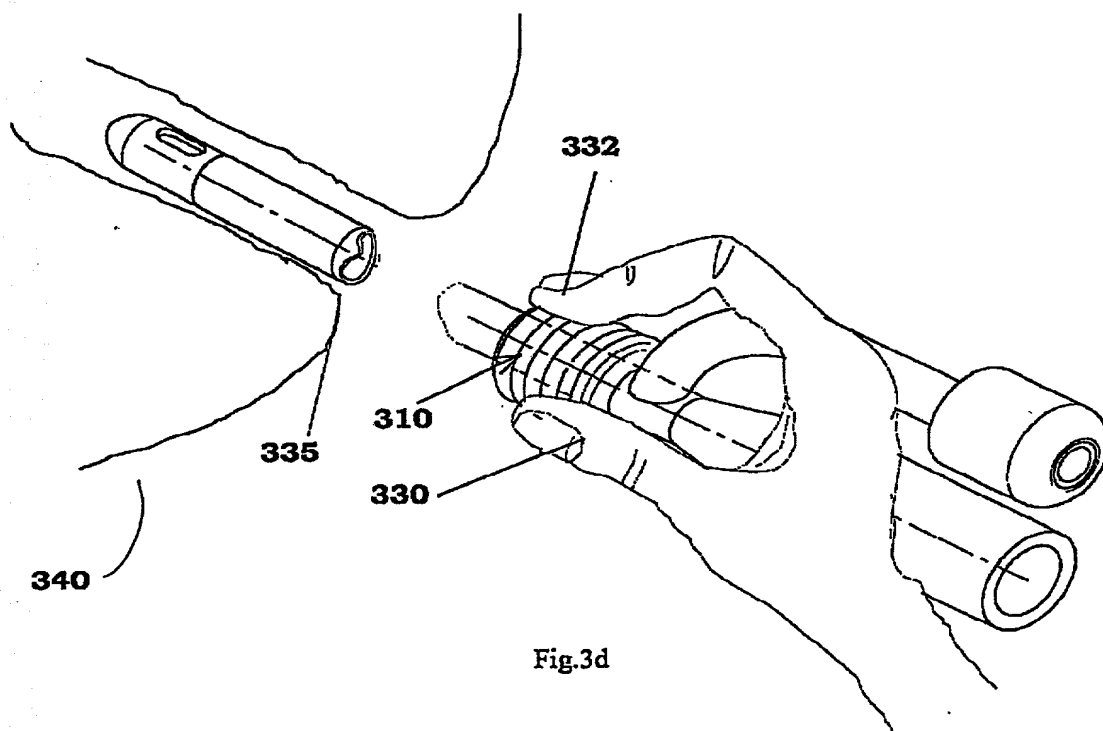


Fig.3d

20250720 14:04:00

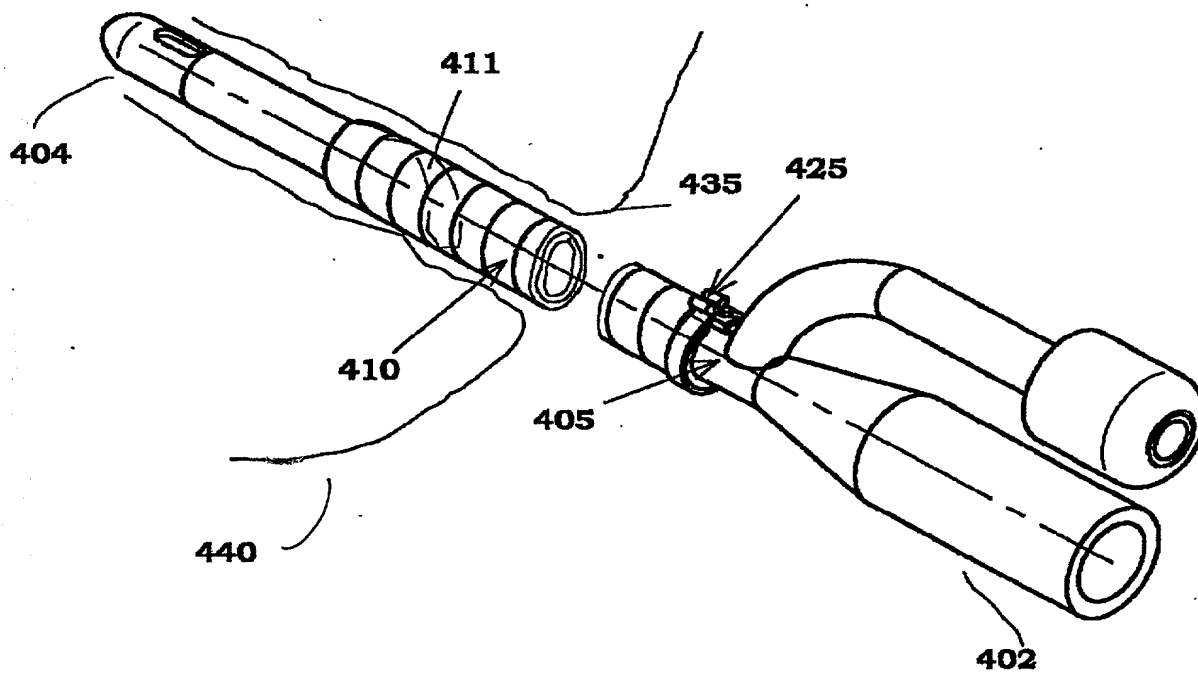
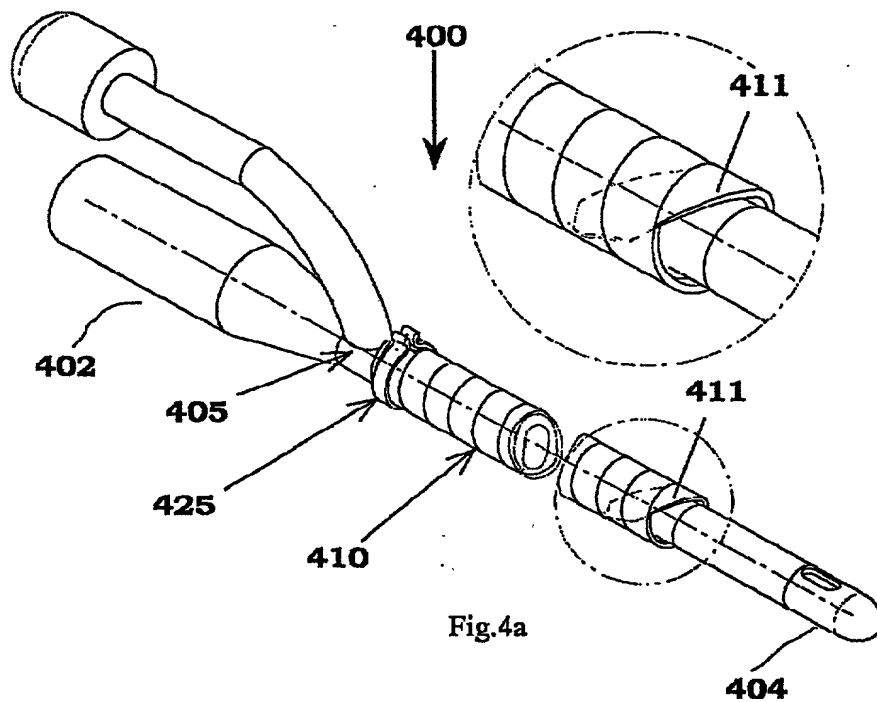


FIG. 5a

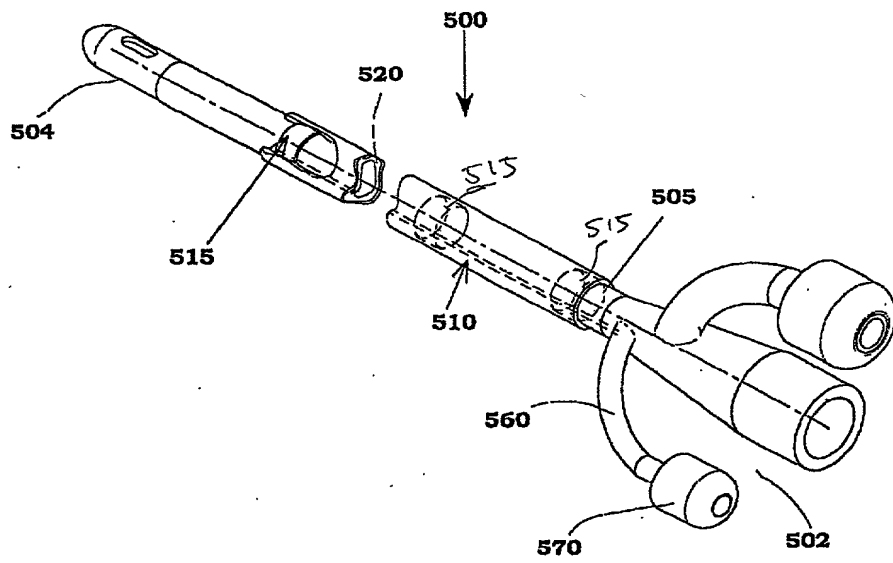


Fig. 5a

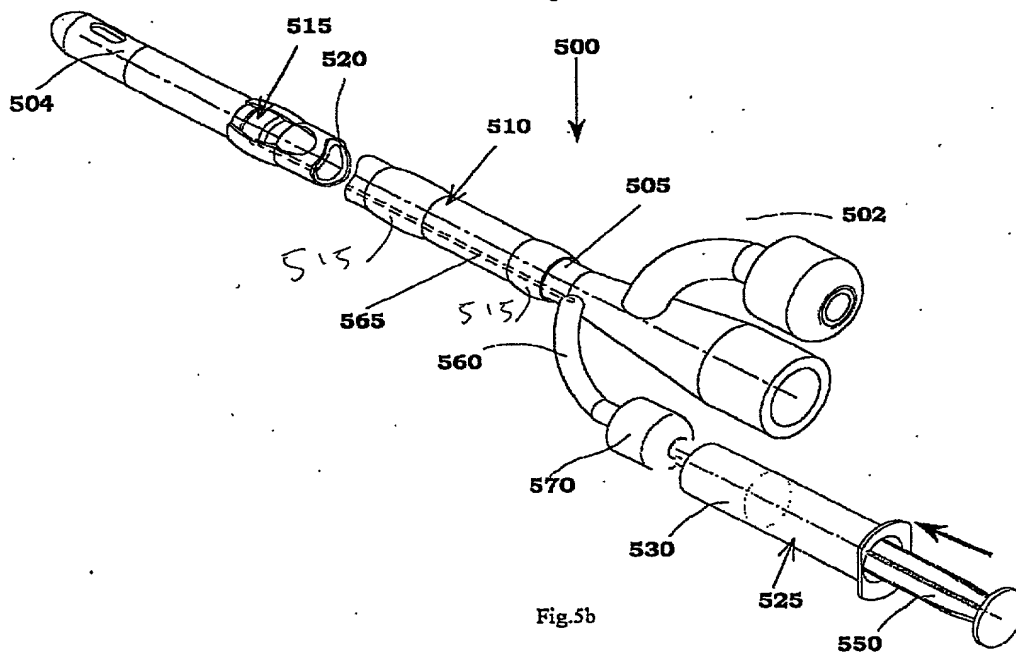


Fig. 5b



20250401 100400

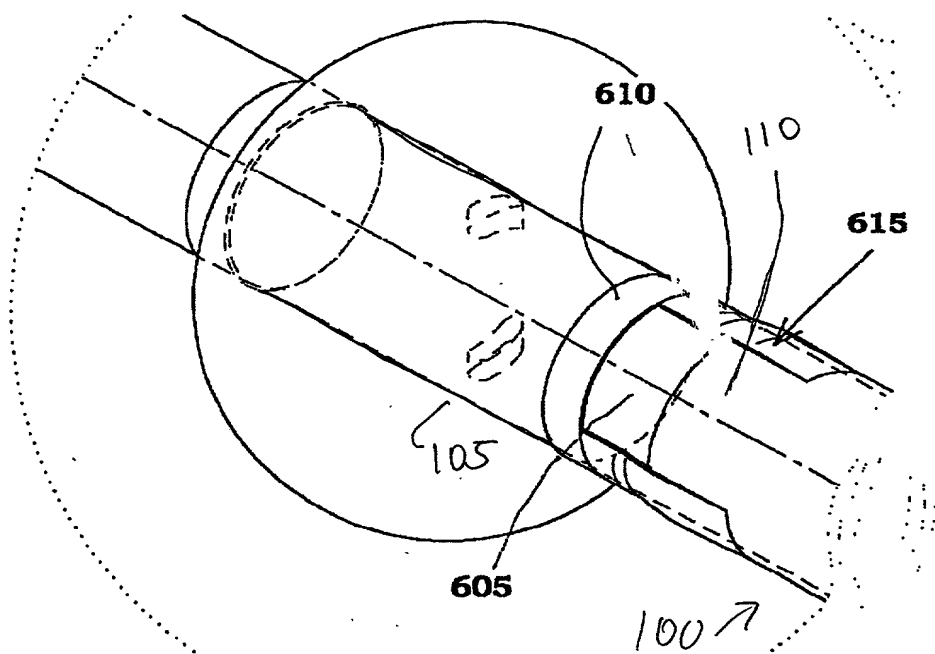


Fig.6

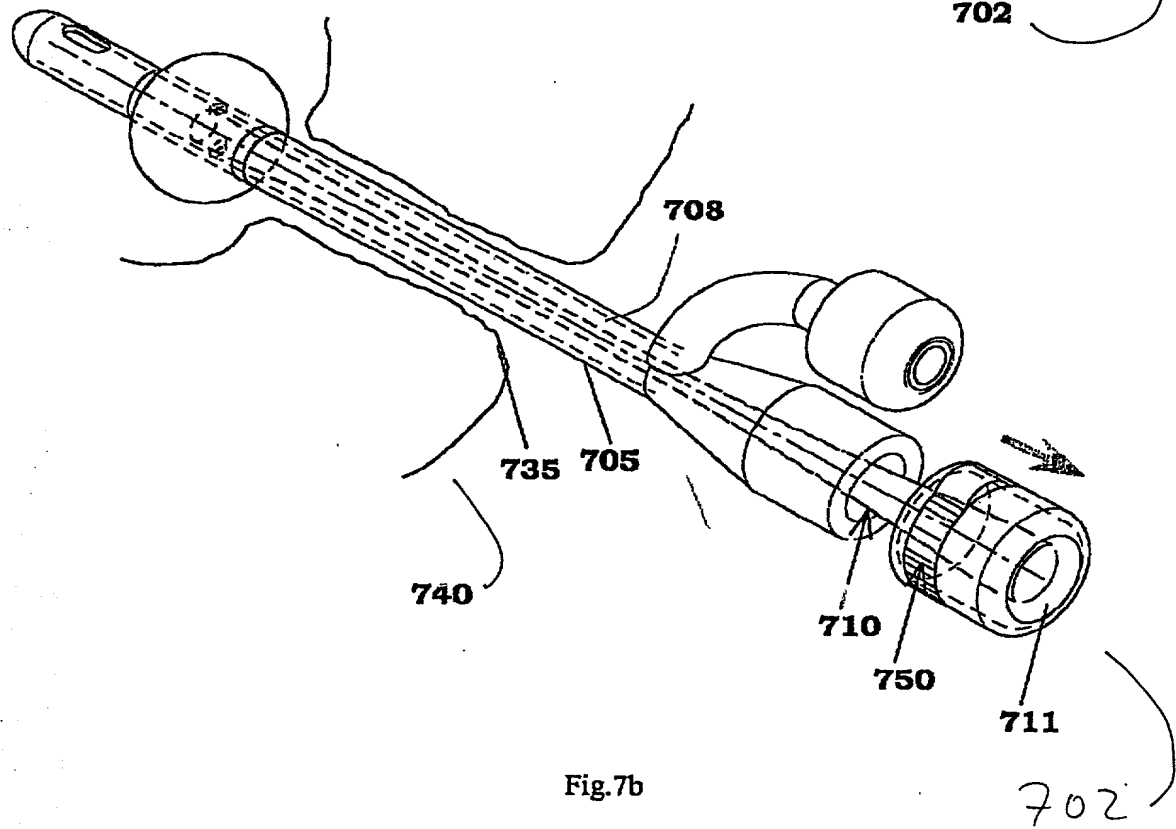
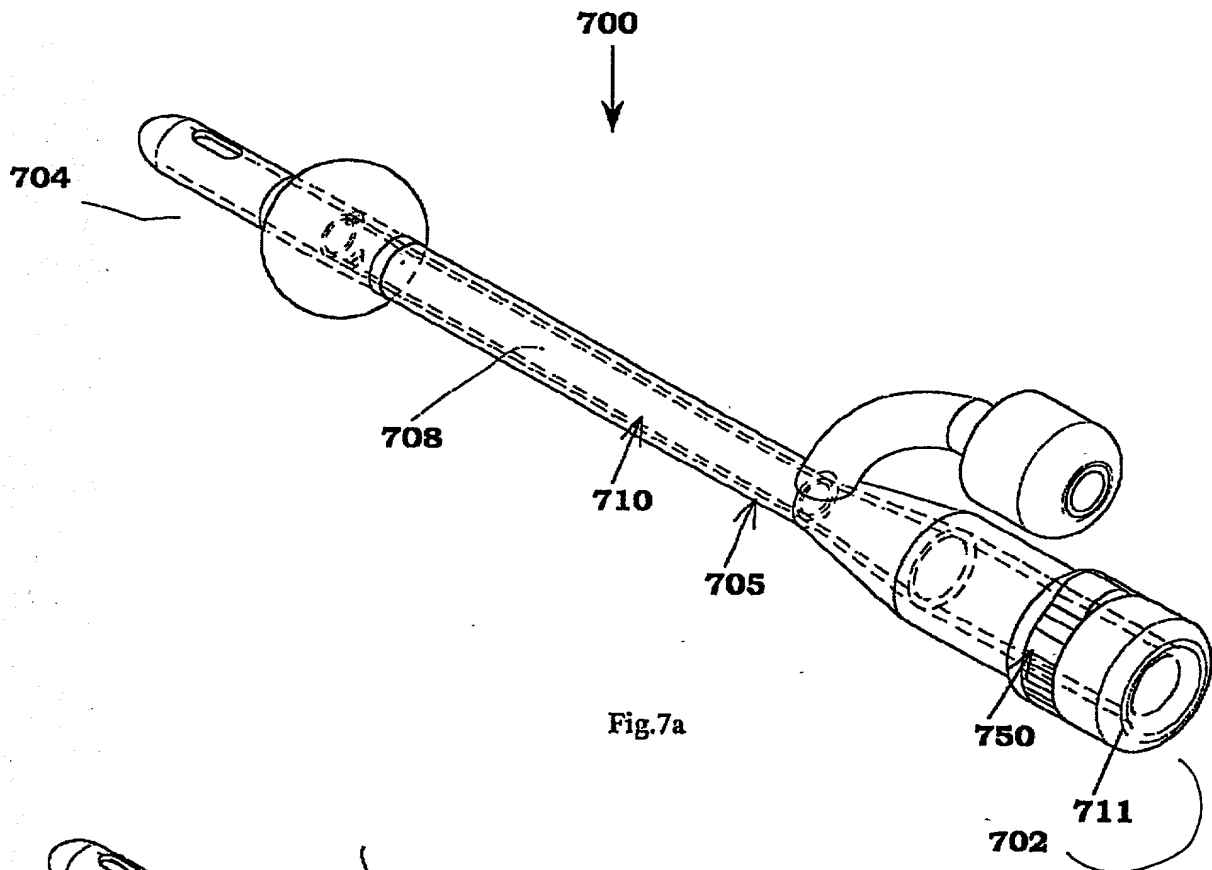
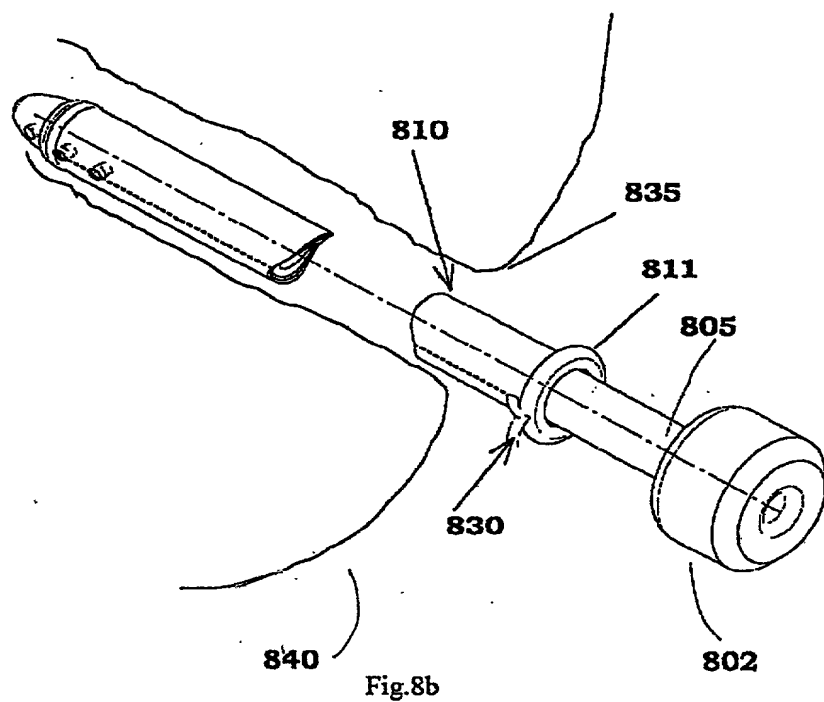
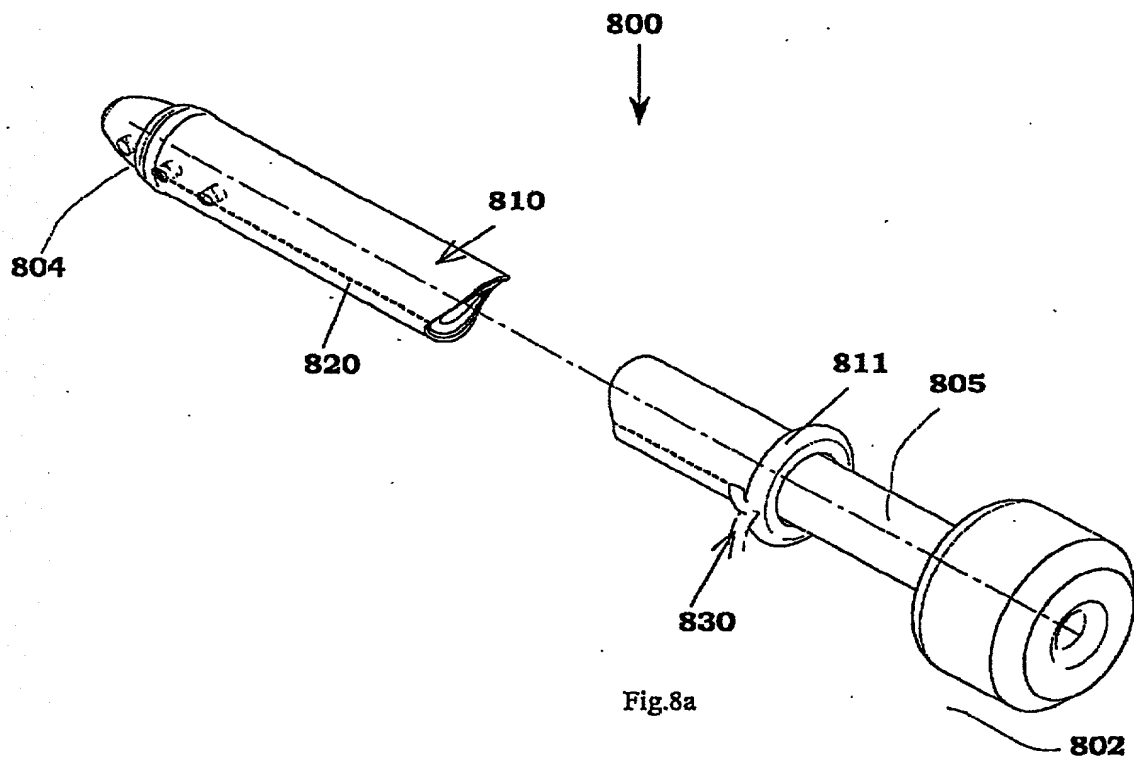
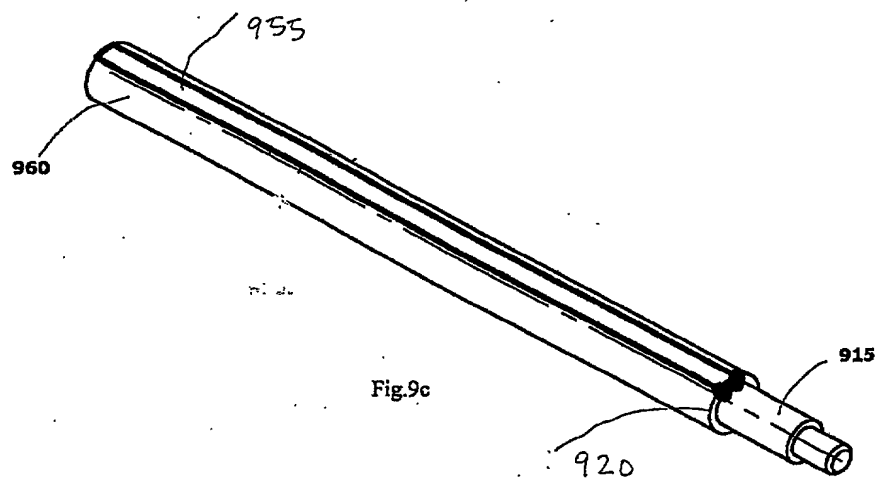
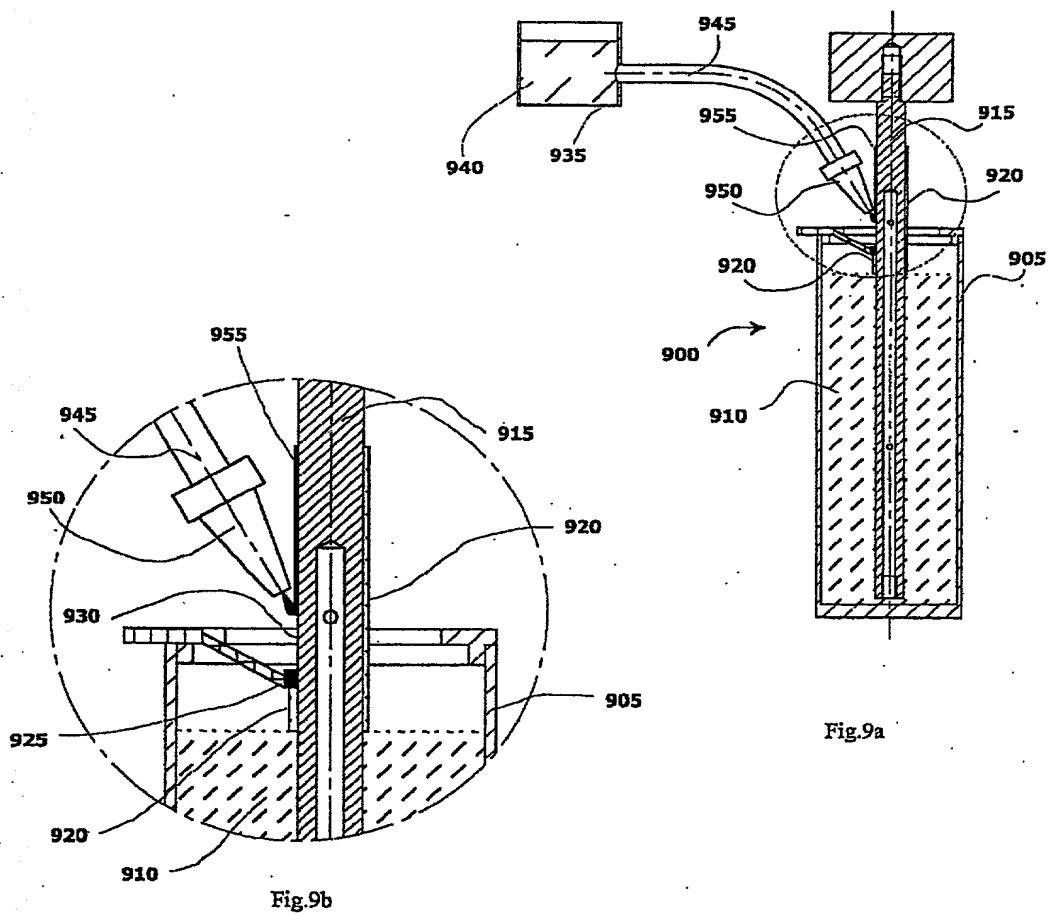


FIG. 8a





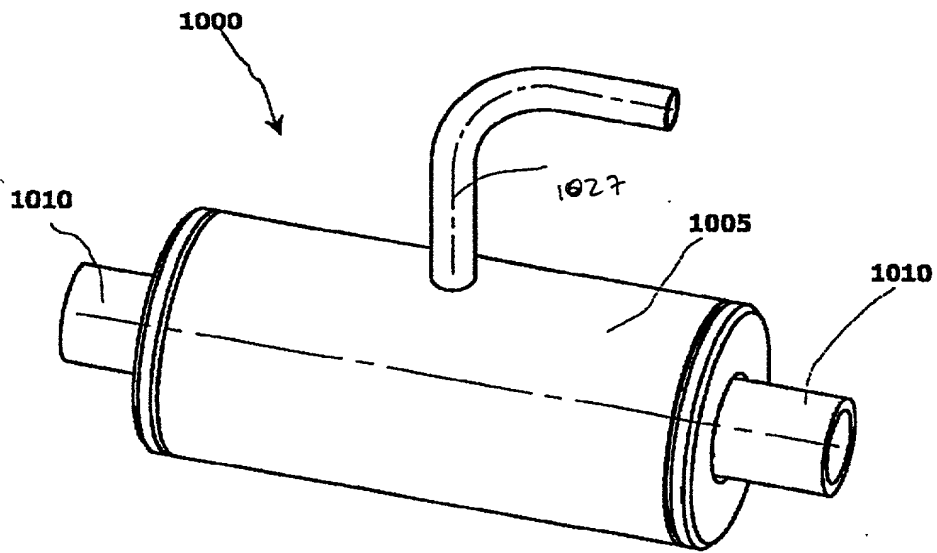


Fig. 10a

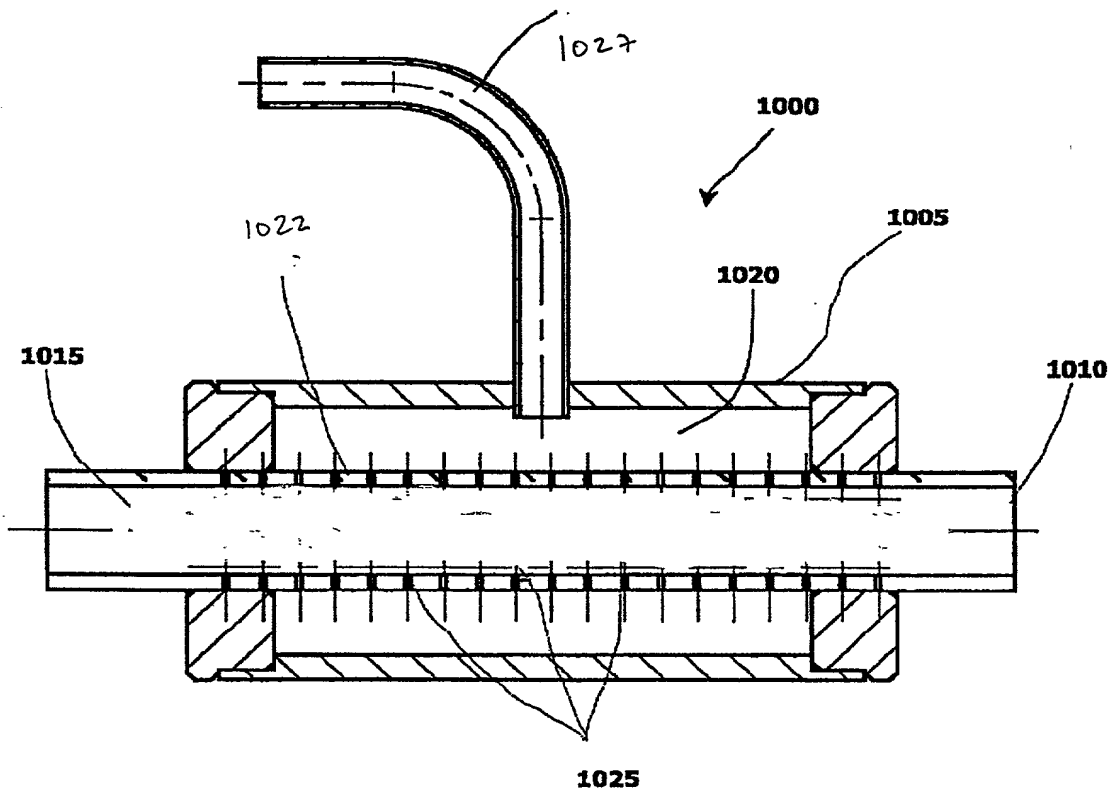


Fig. 10b

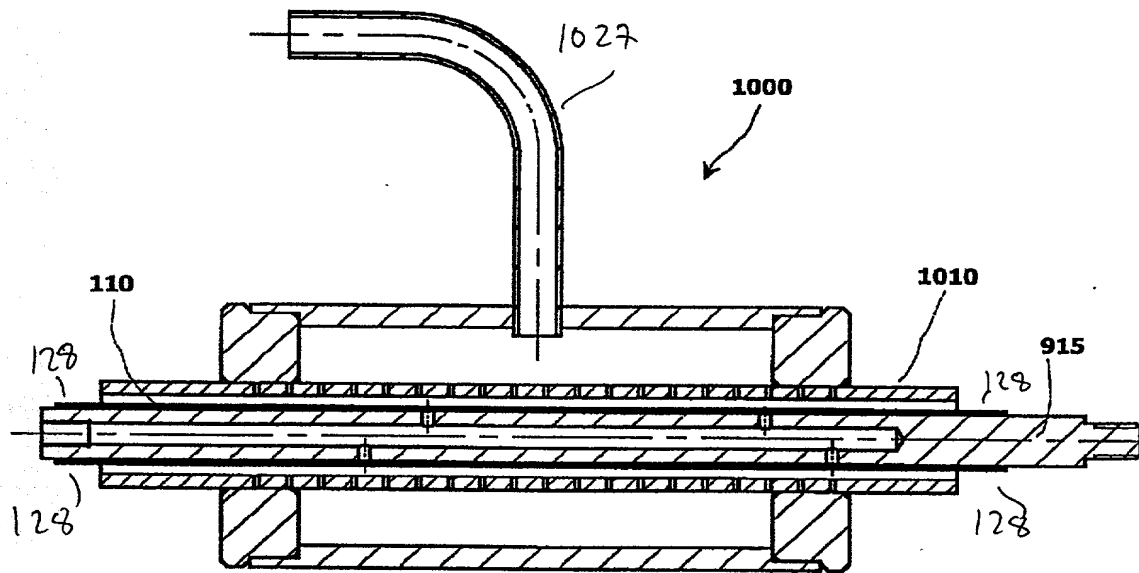


Fig.10c

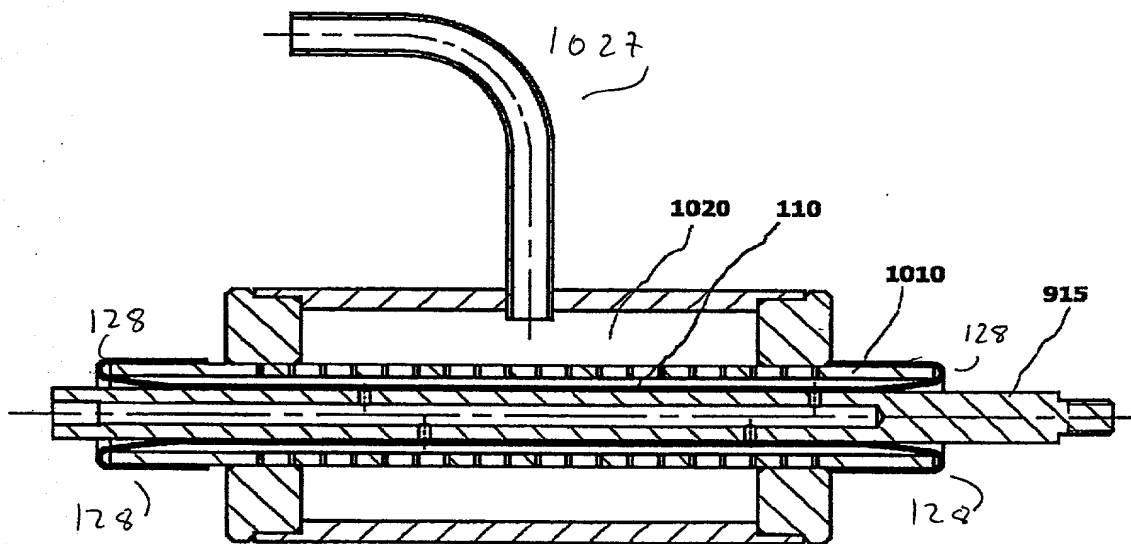


Fig.10d

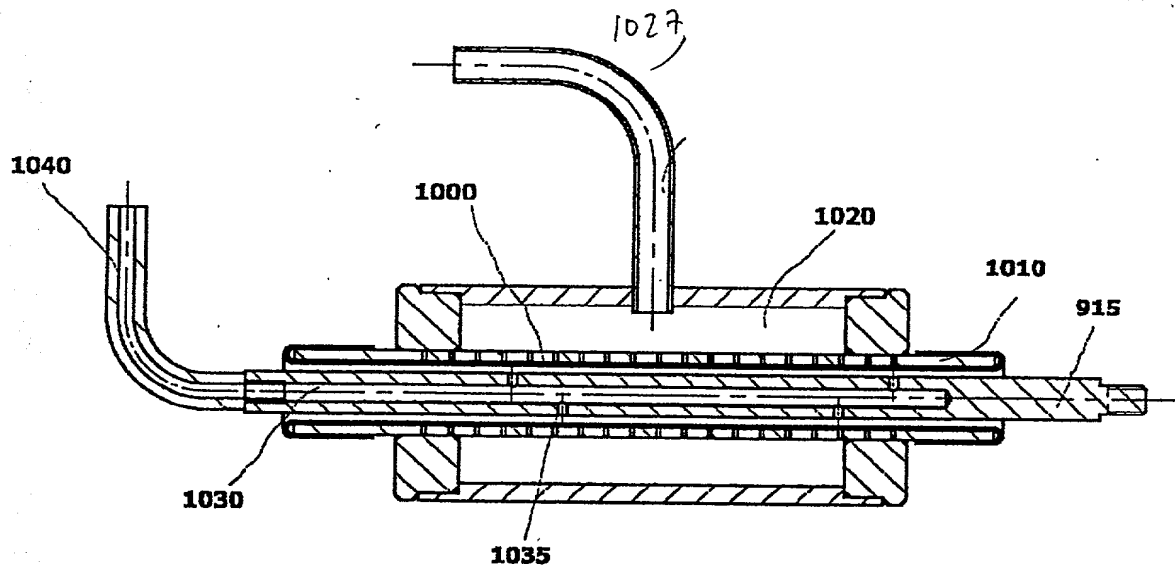


Fig. 10e

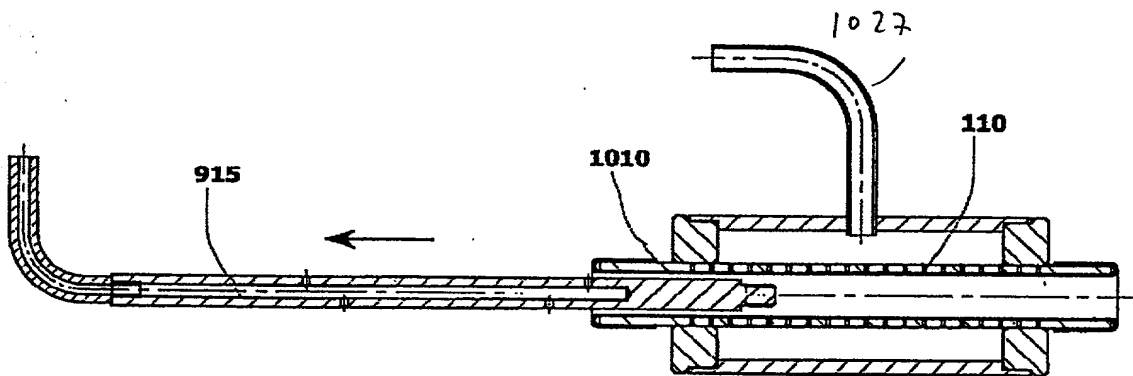


Fig. 10f

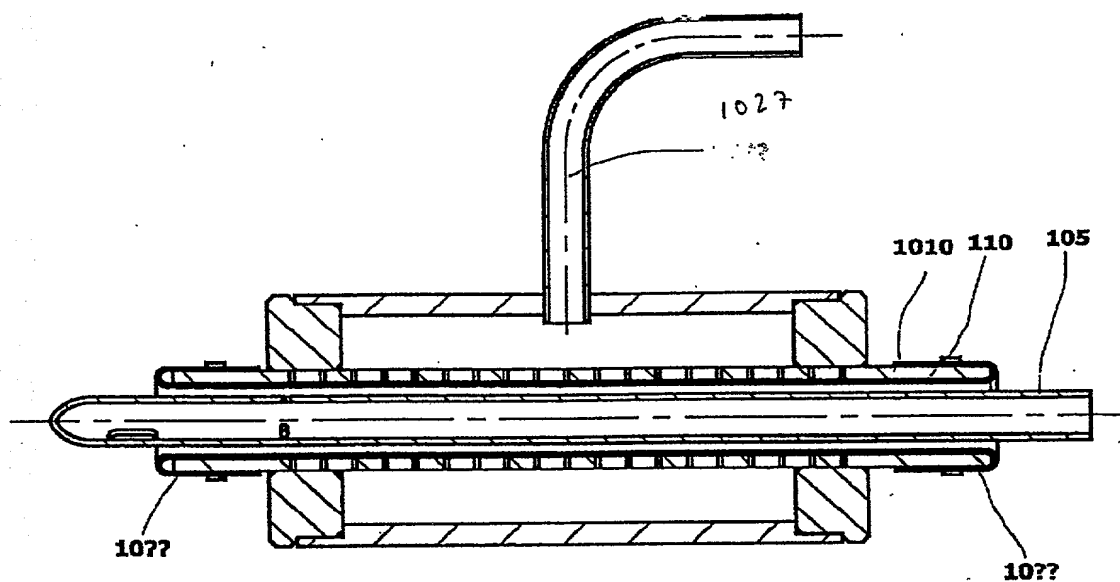


Fig.10g

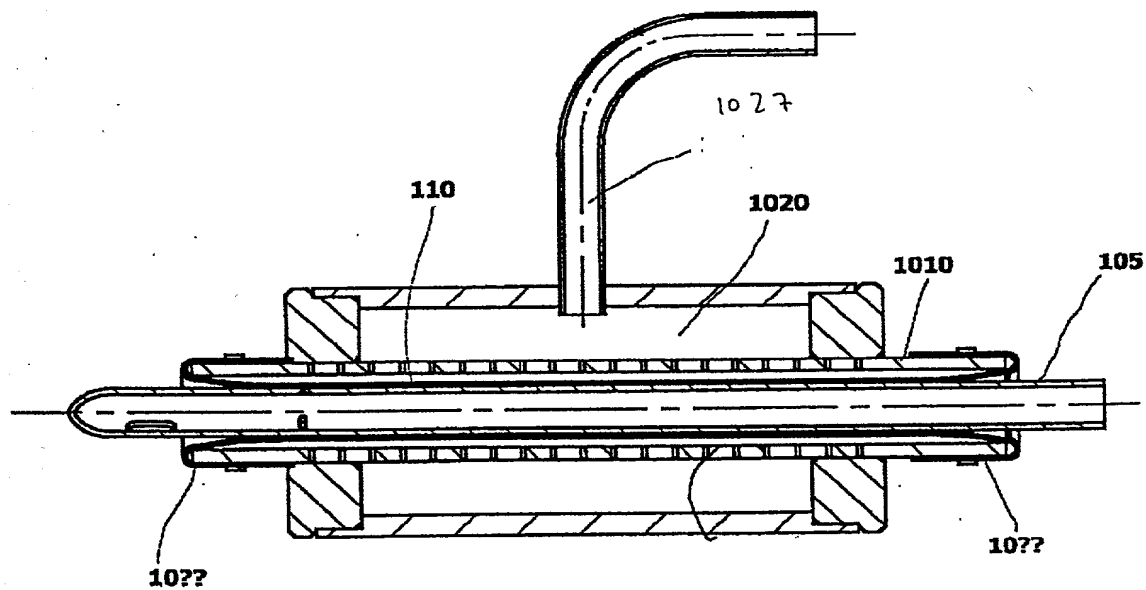


Fig.10h